First Steps Example



VERSION 2023

ReliaSoft

© 1992-2023 Hottinger Bruel & Kjaer UK Ltd ("HBK UK Ltd"), at Technology Centre, Advanced Manufacturing Park, Brunel Way, Catcliffe, Rotherham S60 5WG. HBK UK Ltd is an affiliate of Hottinger Bruel & Kjaer Inc. ALL RIGHTS RESERVED.

This license agreement ("License Agreement") sets forth the terms and conditions that govern the distribution and use of the HBK UK Ltd software documentation (the "HBK Software Documentation"), including any and all derivative works. Any unauthorized distribution or use of the HBK Software Documentation is strictly prohibited.

Licensee hereby acknowledges and agrees to the following terms and conditions of this License Agreement for its use of the HBK Software Documentation:

HBK UK Ltd grants the Licensee who accepts and abides by the terms of this License Agreement a non-exclusive, non-transferable, royalty-free, and revocable license to the HBK Software Documentation. Unless otherwise indicated, all HBK Software Documentation are copyrighted and are the property of HBK UK Ltd or, where applicable, the relevant member of HBK UK Ltd's corporate group. They are licensed to you and for your use only as an individual who has purchased the software ("Licensee"). Notwithstanding this License Agreement, the Licensee shall not have a license to the trademarks, logos, or any other intellectual property of HBK UK Ltd and/or its affiliates or Licensor(s).

Licensee may print a single copy of the HBK Software Documentation for his/her reference. Licensee may reprint the HBK Software Documentation, as needed, if the original printed copy is damaged and/or destroyed.

Except as provided above, no part of the HBK Software Documentation, either text or image, may be used for any purpose other than Licensee's own personal use and reference as a learning aid. Therefore, the reproduction, modification, creation of derivative works, storage in a retrieval system, or retransmission, in any form or by any means, electronic, mechanical or otherwise, for reasons other than Licensee's personal use, is strictly prohibited.

Certain photos and images in the HBK Software Documentation are used under non-transferable licenses obtained by HBK UK Ltd and/or its affiliates and are owned by its Licensor(s) ("Licensor"). Images depicting photos of actual persons are licensed to HBK UK Ltd and/or its affiliates and the signed model releases for these images are on file with the Licensor(s). HBK UK Ltd makes no copyright claims on these images. All ownership and intellectual property rights to the HBK Software Documentation are reserved by either HBK UK Ltd and/or its affiliates or its Licensor(s).

DISCLAIMER: THE HBK SOFTWARE DOCUMENTATION IS PROVIDED "AS IS" WITHOUT WARRANTIES OF ANY KIND, EITHER EXPRESS OR IMPLIED,

INCLUDING, BUT NOT LIMITED TO: 1) ANY IMPLIED WARRANTIES OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE, OR NON-INFRINGEMENT OF INTELLECTUAL PROPERTY; 2) ANY WARRANTY THAT THE HBK COURSE MATERIALS WILL CONFORM TO SPECIFICATIONS; 3) ANY WARRANTY THAT THE WORK WILL BE ERROR FREE OR VIRUS FREE. IN NO EVENT SHALL HBK UK LTD, ITS AFFILIATES, DISTRIBUTORS, CONTRACTORS, AGENTS, AND ITS LICENSOR(S) BE LIABLE FOR ANY DAMAGES, INCLUDING, BUT NOT LIMITED TO, DIRECT, INDIRECT, SPECIAL OR CONSEQUENTIAL DAMAGES, ARISING OUT OF, RESULTING FROM, OR IN ANY WAY CONNECTED WITH THE HBK SOFTWARE DOCUMENTATION, WHETHER OR NOT BASED UPON WARRANTY, CONTRACT, TORT, OR OTHERWISE, WHETHER OR NOT LOSS WAS SUSTAINED FROM, OR AROSE OUT OF THE RESULTS OF, OR USE OF, THE HBK SOFTWARE DOCUMENTATION. LICENSEES AGREE TO WAIVE ANY AND ALL CLAIMS AGAINST HBK UK LTD, ITS AFFILIATES, DISTRIBUTORS, CONTRACTORS, AGENTS, AND ITS LICENSOR(S), AND SHALL INDEMNIFY, DEFEND AND HOLD HARMLESS HBK UK LTD, ITS AFFILIATES, DISTRIBUTORS, CONTRACTORS, AGENTS, AND ITS LICENSOR(S) FOR ANY AND ALL LIABILITIES, CLAIMS, DEMANDS, DAMAGES, EXPENSES OR LOSSES THAT MAY ARISE FROM THE LICENSEE'S USE OR DISTRIBUTION OF THE HBK SOFTWARE DOCUMENTATION, INCLUDING ANY LIABILITIES OR DAMAGES FROM DERIVATIVE WORKS OR OTHER PRODUCTS BASED ON, OR RESULTING FROM, THE USE THEREOF.

This License Agreement is subject to change without notice and does not represent any commitment on the part of HBK UK Ltd and/or its affiliates to the Licensee, including any commitment to maintain or update the HBK Software Documentation. The names of companies, products, people, characters, and/or data mentioned in the HBK Software Documentation are not intended to represent any real individual, company, product or event, unless otherwise noted. Any rights not expressly granted herein are reserved for HBK UK Ltd.

TRADEMARKS:

ReliaSoft, Weibull++, BlockSim, Lambda Predict, XFMEA, RCM++ and XFRACAS are all trademarks of Hottinger Bruel & Kjaer Inc.

GlyphWorks, VibeSys, DesignLife and the nCode logos are all trademarks of HBK UK Ltd.

Other product names and services identified in the HBK Software Documentation are trademarks belonging to their respective trademark holders, and are used for illustration purposes. Their use in no way conveys an endorsement or other affiliation with HBK UK Ltd and/or its affiliates. This License Agreement is subject to change without notice and does not represent any commitment on the part of HBK UK Ltd and/or its affiliates to the Licensee, including any commitment to maintain or update the HBK Software Documentation. The names of companies, products, people, characters, and/or data mentioned in the HBK Software Documentation are not intended to represent any real individual, company, product or event, unless otherwise noted. Any rights not expressly granted herein are reserved for HBK UK Ltd.

Introduction

This example provides a quick introduction to the RCM++ software by allowing you to experiment with the application's data management, analysis and reporting features. For this example, you will work with a project that contains part of an RCM analysis for a standard pump. The analysis was performed using the RCM logic diagrams published in the SAE JA1012 guidelines. These instructions were prepared with RCM++ 2023 but you can perform the same steps in previous versions back to Version 9. The appearance of a few icons and interfaces will vary slightly.

A Note About RCM Terminology in the Software: RCM++ combines RCM capabilities and FMEA capabilities together in the same software interface. Although there are many similarities between the two analysis methodologies, there are some basic differences in the terminology that affect the application interface. Note the following:

FMEA and Functional Failure Analysis: Regardless of whether you are performing an RCM analysis or an FMEA, all of the information related to the functions and failure modes will be displayed in the FMEA tab of the Analysis panel, and you will use the commands in the FMEA tab of the ribbon to manage this information. In other words, the term "FMEA" is often used within the software interface in place of "functional failure analysis."

Functional Failures, Failure Modes and Causes: Although the property names within the software are fully configurable to fit the specific analysis terminology used by your organization, the ribbon commands, icons and window names are not. When a name is not configurable, the term "Failure" is used for the second level in the analysis hierarchy and "Cause" is used for the fourth level. If you are performing a functional failure analysis, you might refer to these levels as the "Functional Failure" and "Failure Mode."

Open an Existing Database

If you haven't started RCM++ already, browse for and select the RCM++ application in the Windows Start menu.

When you launch RCM++, the Backstage view (File tab) is the first view you will see. This Backstage view provides a quick way to create and open databases. In ReliaSoft desktop applications, *standard databases* are Microsoft Access® databases. These are easy to create and maintain without any special IT infrastructure or support, but there are limitations to the amount of data they can store and the number of users who can access the repository simultaneously. *Enterprise databases* require implementation of Microsoft SQL Server® or Oracle® (which require separate licensing, support and maintenance), but are a more robust platform that can store much more analysis information in the same database and support access by many more simultaneous users.

For this example, you will use a standard database that is installed with the software (called "RCM23_Examples.rgz23") that contains several sample projects. (If you are using Version 2022, the file is called "RCM22_Examples.rgz22," and so on.) To access this file, choose **File > Help**, click **Open Examples Folder**, then browse for the file in the RCM sub-folder.

Tip: To preserve the integrity of the shipped example files, the software creates a copy of the file each time you access a repository in the Examples folder. The copy has the same name as the original file and is saved in the default documents folder for your computer (e.g., My Documents\ReliaSoft\Files). Use the copy to work on the example projects and save your changes. Any changes you make in the copy will not affect the original file.

View the Project Properties

In all ReliaSoft desktop applications, *projects* give you the flexibility to manage your analyses to fit the particular needs of your organization. You can have one or many projects in the same database.

Every RCM++ analysis within a given project will have the same configurable settings, including the fields that are enabled/disabled in the interface and reports, the rating scales or questions that are available for risk assessment and the options that are available for codified information (such as FEC logic, task selection logic, etc.).

To save time and ensure consistency, these configurable settings can be set automatically based on predefined *profiles* that are managed by authorized users. They can also be viewed or modified directly in each individual project.

• Select the **RCM** - **Pump Analysis with Simulations** project in the Project Manager and choose **Project** > **Management** > **Edit Project Properties** to open the Project Properties window, as shown next.


💩 Edit Pr	oject Properties (Project:	RCM - Pump Analysis wi	th Simulations)		?	×
General	Configurable Settings					
Name						
RCM - Pun	np Analysis with Simulations					
Descriptio	n					
	ject, an abbreviated RCM ana derstand how RCM++ is used					•
Remarks						
	: Example projects are purely ely represent any real physica		ures and functionality	. They are not inten	ded ,	•
Proprietan	y Label					
For Demor	nstration Purposes only - does	not represent specific equip	ment.			1
EMEA Stru	rture	Select	Profile from Library			
	fore Causes		d on SAE RCM (4 Cat	egories)]	•	- /
Project Cat	tegory					
RCM						-
			ABC	ОК	Cano	cel
project Ow	ner: HBM Prenscia					

As can be seen in the **Select Profile from Library** field, the configurable settings in this project are based on the SAE RCM (4 Categories) profile. This predefined profile is shipped with the software and can be used to quickly configure the project to use the data fields and logic diagrams specified in the SAE JA1012 "A Guide to the Reliability-Centered Maintenance (RCM) Standard" guidelines for RCM.

- Now click the Configurable Settings tab. This page provides one way that you can view (and edit) the configurable settings that have been copied into the current project from the predefined SAE profile. (Note that the settings are also accessible when you are working in the project by choosing Project > Management > Configurable Settings or by clicking any of the Configurable Settings icons.)
- As an example, click the View/Edit Settings icon for FEC Logic.

Tasks	
FEC Logic	_
Current Settings	- 🖍
Task Selection Logic	
Current Settings	- 🎤

You can see that the project has been configured to use the 4-category failure effect categorization diagram from the SAE standard.

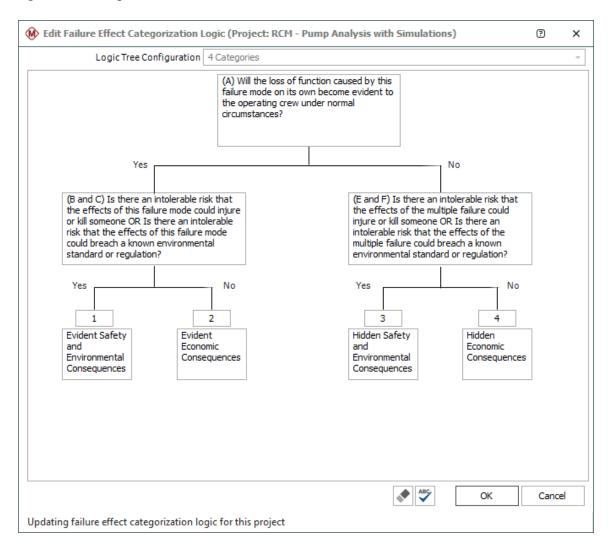

- Click **Cancel** to close the failure effect categorization logic window without saving any changes.
- If desired, you can click the other **View/Edit Settings** icons to see the rest of the configurable settings that have been predefined for this project. When you are finished explor-

ing these settings, click **Cancel** to close the Project Properties window without saving any changes.

Open a Project

With the RCM - Pump Analysis with Simulations project still selected in the Project Manager, open the project either by double-clicking the project name or by choosing Project > Management > Open Project.



The Project window is the main interface that you will use to perform your analyses. It is divided into two panels, as shown next.

RCM - Pump Analysis with Simulations	0						
📩 System Hierarchy				Properties A Risk Disco	overy F FMEA		
Name		<u>A</u> :	F	Property Name	Value	^	
🗆 💼 Pump_Centrifugal_MotorDrive		2	F	Identifiers			
Impeller and shaft sub- assembly			F	Image 🗾			
Key - Coupling				Name	Pump_Centrifugal_MotorDrive		
Lock nut Assembly - shaft				Category 🕨	No Category		
Key - Impeller				Part Number			
Slinger Ring - water				Supplier			
Wear plate				Application			
System Panel				Description		Analy	/sis
				Keywords 🕨	0		
				Other Item Properties			
				Operation			
				Operating Time	20000 (hr)		
				Current Age	0 (hr)		
Hierarchy	View			Duty Cycle	1		
T Incrarcity T Filtered	i view			Maintenance Group		¥	

(If not all of the properties shown in this image are visible on your computer, you can show them by clearing the **Hide reliability nodes on item properties** option on the Settings page of the Application Setup window.)

The System panel displays the system hierarchy, which includes all items that have been defined in the project. The Analysis panel displays information and analyses associated with the item that is currently selected in the hierarchy. Depending on your preferences, these panels can be displayed side-by-side, or with one panel above the other.

View the Item Properties

The Properties tab in the Analysis panel displays the item properties fields that are enabled for the current project, along with some settings that can be used for reliability calculations (if desired) and information about when the item record was created and last updated.

You can click inside any field with blue text to edit it. Fields shown in italics cannot be edited, either because they are populated by the application or because they are based on inputs that you make elsewhere in the software.

- If the item properties are not already displayed, click the **Properties** tab at the top of the Analysis panel.
- As an example, click inside the Part Number field and type PN9999, as shown next.



• If desired, you can edit any of the other item properties. When you are finished exploring these properties, proceed to the next section.

View the Equipment Selection

RCM++ supports two configurable methods for evaluating potential risk and selecting which items will receive further analysis. The Risk Discovery tab displays the questions or ratings that have been defined for the current project. For this example, the project uses a set of four yes/no questions to select which equipment should receive RCM analysis.

Note: A project can also be configured to use the Risk Ranking method for equipment selection (which uses a set of configurable rating scales). This is determined by the option that is selected in the Risk Discovery area on the Configurable Settings tab of the Project Properties window (Use Risk Discovery Questions or Use Risk Discovery Ratings).

• Click the **Risk Discovery** tab in the Analysis panel to view the equipment selection analysis for the pump.

RCM - Pump Analysis wi	th Simulation	S	0									
🕂 System Hierarchy	F, FMRA							Properties	A Risk Discovery	FFMEA		
Name		1	Ø		<u>_</u> :	F	1	Label	Question		/ Response	/ Comments
Pump_Centrifugal_N Impeller and sha assembly				4	2	F		Safety	Could failure affect safety other hazardous consequ		No	
Key - Couplin	-							Detectability	Could failure be undetect likely to be detected duri operation?		No	
Key - Impeller Slinger Ring -								Operational	Could failure have signific operational impact?	cant	Yes	Failure could interfere with the performance of othe equipment in the manufacturing line.
								Economic	Could failure have signific economic impact?	cant	Yes	Failure could result in lost production.
🕂 Hierarchy	🕈 Filter	ed V	'iew					✓ Mark item for	more detailed analysis			

In this utility, you can click inside the Response column to toggle the answer between "Yes" and "No." The label will be displayed in green to indicate a "No" answer (not critical) or in red to indicate a "Yes" answer (critical). If desired, the team can use the Comments column to record any additional information relevant to the responses.

- To see the colors change, click inside the Response column to toggle both of the current "Yes" answers to "No." You can see that the **Mark item for more detailed analysis** check box is cleared automatically and the risk discovery icon in the System panel changes from red to green.
- Now click the check box to select the option again. You can see that the risk discovery icon in the System panel changes back to red. In other words, the application will automatically


update this icon based on your answers to the selection questions, but you have the option to override this setting if desired.

• Before proceeding to the next section, click inside the Response column again to toggle the Operational and Economic answers back to the original "Yes" answers.

View the Functional Failure Analysis

The FMEA tab in the Analysis panel allows you to view/edit the functional failure analysis for the currently selected item.

• Click the **FMEA** tab to view the functional failure analysis for the pump. There are now four tabs at the bottom of the Analysis panel. Each tab displays the analysis information in a different way to facilitate data entry and decision making.

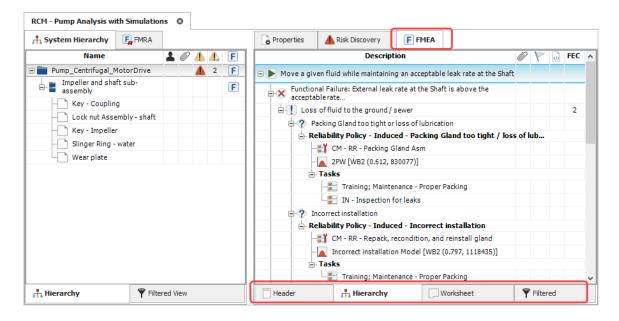

The Hierarchy View

The hierarchy view displays the analysis records in a hierarchical tree, which tends to be good for viewing a lot of information in a small amount of space. It can be especially useful when copying and pasting data or when scanning the analysis to find a particular section.

- If the hierarchy view is not already displayed, click the Hierarchy tab to view it.
- Double-click the "Move a given fluid..." function record at the top of the tree. The function properties window will appear, as shown next.

M Edit Function					×
Home Navigate					
Add Function Add Failure	Add Effect Add Cause	Configurable Settings	Spelling Attachments Change Log Cools		
Function					
Function	Move a given fluid while	maintaining an a	acceptable leak rate	at the Shaft	
Name	*				
Keywords 🗾 📢					
Associated Records					
Item	Pump_Centrifugal_Motor	Drive			
🖃 History 🔯					
Created By					
Date Created	4/3/2012 11:44 AM				
Last Updated By 💄					
Last Updated	4/3/2012 11:44 AM				
Function					
			ОК	Cance	<u>!</u>
Editing function properties					.::

- With the properties window still open, click the first functional failure ("Functional Failure: External leak rate at the Shaft...") in the FMEA hierarchy. You can see that the window updates automatically to display the properties for the record that is currently selected.
- If desired, you can continue clicking different records in the hierarchy to view their properties. Note that this approach works for any record type except tasks, which have a specialized interface to facilitate integration with other ReliaSoft applications (such as BlockSim). When you are finished exploring, click **Cancel** to close the properties window without saving any changes.
- Now create a new branch in the hierarchy by right-clicking the "Move a given fluid..." function and choosing **Add Function** from the shortcut menu.



• In the properties window, type "New Function" in the **Function** field and then click the **Add Failure** icon at the top of the window.



• The properties window is now prepared to define a new functional failure. In the **Func-tional Failure** field, type "New Functional Failure" and then click the **Add Effect** icon.



• Now you can define a new effect. In the **Effect** field, type "New Effect" and then click the **Add Cause** icon.



• Now you can define a new failure mode. In the **Failure Mode** field, type "New Failure Mode" and then click **OK** to close the properties window.

You can see that there is a new branch at the bottom of the hierarchy with the new records you just created.

New Function		
- New Functional Failure		
- New Effect		
Ė-?∕ New Failure Mode		
🚽 Reliability Policy - Default (Not Set)		
– Tasks		

The Worksheet View

The worksheet view provides an alternative way to view/edit the same analysis information displayed in the hierarchy view. This view allows you to type directly into the worksheet cells and tab through the analysis as you would in a spreadsheet application such as Microsoft Excel®.


• To give more space in the Analysis panel before switching to the worksheet view, first choose View > Workspace Layout > Hide System Panel.



• Now click the **Worksheet** tab at the bottom of the Analysis panel.

R	CM - Pump Analysis with Simulatio	ons ©				
G	Properties 💧 Risk Discovery	F FMEA				
	Function		Functional Failure		Effect	Failure Mode
1	Move a given fluid while maintaining an acceptable leak rate at the Shaft	above the acce	lure: External leak rate at eptable rate ode: Packing worn	the Shaft is	Loss of fluid to the ground / sewer	Packing Gland too tight or loss of lubrication
2						Incorrect installation
3						Wear Out - Normal wear
4		the acceptable	lure: Leak rate at the Sha e rate ode: Packing mis-adjuste		Packing prematurely worn	Packing bolts over tightened
5		Functional Failure: Catastrophic failure of the Shaft Seal Failure Mode: Seal/Packing blowout			Process impact and Loss of fluid to the ground / sewer	Induced - Gland Follower corrosion / failure
6						Induced - Gland Follower stress / failure
7	New Function	New Functiona	al Failure		New Effect	New Failure Mode
	Function	l	0 Attachments			
	Header	🕂 Hierarchy		Workshe	eet	F iltered

• Double-click inside the first function description. You can see that the cell switches from "select mode" (with a blue background) to "edit mode" (with a white background and a blinking cursor so you can modify the text).



• Press ENTER. Note that the blinking cursor now appears in the second function description. Press ENTER again and the application will automatically create a new row so that you can type a new function description at the bottom of the worksheet, as shown next.

Function
Move a given fluid while maintaining an acceptable leak rate at the Shaft
New Function

• This time, instead of typing the function description, you can use the Select Existing utility to reuse text that is already stored in the database. While the cell is in "edit mode," click the **Select Existing** icon.



- In the Select Existing window, look at the Project Filter, Item Filter, Record Filter and Phrase Sets drop-down lists. These lists allows you to specify the source(s) for the list of existing descriptions that you can select from.
- Look in the list of descriptions and double-click any existing description from the list. This automatically enters the selected text into the worksheet cell. This convenient feature is available for text fields throughout the application.
- If desired, you can continue to explore the worksheet view by adding and editing records. When you are finished, proceed to the next section.

The Filtered View

The filtered view allows you to generate sortable lists of different types of records. For example, you can view a list of all failure modes in the analysis, all tasks sorted by type, etc.

- Click the **Filtered** tab at the bottom of the Analysis panel.
- From the **Filter By** drop-down list at the upper right corner, choose **Causes**. The Analysis panel will change to display all of the failure modes that have been defined in the current analysis (sorted in alphabetical order by default).

G	Properties	🛕 Risk Discovery	F FMEA					
					Filter By	Causes		•
				Failure Mode			Ø	9
1	? Incorrect in:	stallation						
2	🥐 Induced - G	land Follower corrosior	ı/failure					
3	🥐 Induced - G	land Follower stress / fa	ailure					
4	? New Failure	Mode						
5	Packing bol	ts overtightened						
6	Packing Gla	nd too tight or loss of lu	brication					
7	🥐 Wear Out -	Normal wear						
F	Header		Hierarchy	Worksheet	Filtered			_

• You can sort the records by clicking any of the column headers. You can also double-click any record to open its properties window.


- If desired, you can continue to explore the filtered view by changing the filter or sorting by different columns. When you are finished, click the **Hierarchy** tab to return to the hierarchy view.
- To show the System panel again, choose View > Workspace Layout > Split Panels.



View the Failure Effect Categorization

The FEC column displays the failure effect categorization for each failure effect. (If the FEC column is not displayed on your computer, right-click a column header in the FMEA and choose **Customize Columns**. In the Customize Columns window, select the **FEC** column check box, and then **click** OK.)


• With the FMEA hierarchy displayed, double-click inside the FEC column for the "Loss of fluid to the ground / sewer" effect.

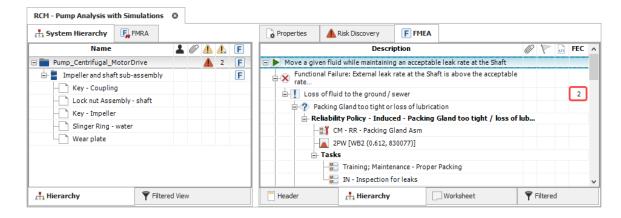

The Failure Effect Categorization window displays the FEC logic diagram that is being used for all RCM analyses in the current project. There are two ways to select the category:

- 1. Answer each individual question until a category is highlighted.
- 2. Select a category directly from the Category drop-down list in the bottom right corner.

If desired, you can use the text fields on the right side of the window to record any additional information relevant to a particular response (use the **Answer** fields) or the categorization overall (use the **Remarks** field). The following picture shows the failure effect categorization that has been performed for the "Loss of fluid..." effect.

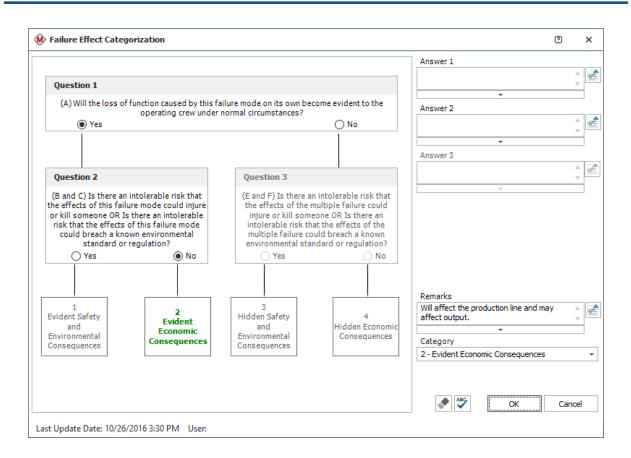


- To see the categorization change, select **No** for Question 1. When Question 3 becomes enabled, **select** No again. You will see that the "4 Hidden Economic Consequences" category is now highlighted.
- To return to the original categorization, choose **2 Evident Economic Consequences** from the **Category** drop-down list.
- Click **Cancel** to close the window without saving any changes.

Assign the Reliability and Corrective Maintenance Policies

For this project, the team is using a combination of RCM design logic and availability/cost calculations to select the appropriate maintenance strategies. As an example, you can complete the sample analysis by entering the data for the "Wear Out - Normal wear" potential failure mode.

• Right-click the **Reliability Policy** node under the "Wear Out - Normal wear" failure mode and select **Apply Existing URD**.

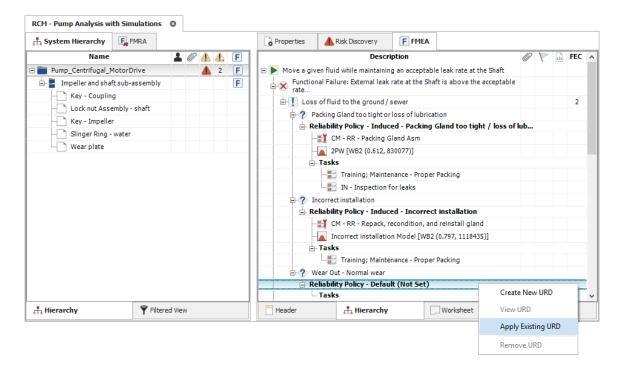

A universal reliability definition (URD) is a resource that describes a set of reliability and maintainability properties. It can be shared by all analyses in a given project. You have the option to create these resources as needed while performing an analysis, or select to use resources that have already been defined.

• The Select Resource window displays a list of all the URDs that have already been created for this project. Select **Wear Out - Normal wear** and click **OK**.

ø	B	• 👦 🛱 🔹	56	elect Resource		□ ×
Но	me	Administration				*
Show	w All	Show Only Show Only	w Global		Trace Make Global Usage Selected Resource	
Shov	w All					- + / ×
		URD Name	Failure Model	Failure Model Information	Corrective Task	Scheduled Tasks
Ŧ		RBC	8 8 0	RBC	RBC	8 B C
	0	Broken impeller vane	Broken / chipped impeller vane	WB2 (2.96, 23463)	CM - Replace impeller	Inspect for broken / damaged imp
: 💡	0	Low Risk	Very Low Risk Item	WB2 (1.48, 174994)		
12	۲	Wear Out - Normal wear	Wear Out - Normal - Model	WB2 (3.5, 8500)	CM - RR - Packing Gland Asm	
1	0	Gland Follower corrosion / failure	Gland Follower corrosion - failure	WB2 (3.63, 15850)	CM - RR - Gland Follower	OC-Inspection for corrosion
: 💡	0	Operator error-packing set-up	Operator error - packing set-up	WB2 (0.43, 148132107)	CM - RR - Packing Gland Asm	Training; Maintenance - Proper Pa
2	\bigcirc	Induced - Packing Gland too tight	2PW	WB2 (0.612, 830077)	CM - RR - Packing Gland Asm	Training; Maintenance - Proper Pa
2	\bigcirc	Gland Follower stress / failure	Gland Follower stress failure URD	WB2 (1.55, 125791)	CM - RR - Gland Follower	PM - Gland Follower
2	\bigcirc	Induced - Incorrect installation	Incorrect installation Model	WB2 (0.797, 1118435)	CM - RR - Repack, reconditio	Training; Maintenance - Proper Pa
2	0	Impeller vane wear	Impeller - vane wear	WB2 (1.16, 105891)	CM - Replace impeller	PdM - Track Flow Rate
2	0	Packing Gland too tight / loss of lu	2PW	WB2 (0.612, 830077)	CM - RR - Packing Gland Asm	
•						•
						<u>O</u> K <u>C</u> ancel
URD	Is S	Show Local Resources All				

• When you return to the FMEA hierarchy, you can see that this URD defines the probability of failure for this mode (using a 2-parameter Weibull distribution with Beta = 3.5 and Eta = 8,500 hours) and the unplanned (corrective) maintenance logistics and costs.

🖃 🥐 Wear Out - Normal wear
占 Reliability Policy - Wear Out - Normal wear
📰 CM - RR - Packing Gland Asm
- Wear Out - Normal - Model [WB2 (3.5, 8500)]

• Double-click the "CM - RR - Packing Gland Asm" task to open the Maintenance Task window for the corrective maintenance task, as shown next.

Maintenance Task		
Task Name		
CM - RR - Packing Gland Asm		
	•	
Corrective Properties		1
🗆 🛃 Task Scheduling		
Start corrective task	Upon item failure	•
= 🏠 Basic Repair Properties		
-A Task duration (hr)	Emergency Repack [3]	
🖃 🌉 Teams for task		
- Team (Priority 1)		
E- Crew	Pump EM Crew - \$200/Hr	
Logistic delay (hr)	Crew Response Time [NOR (0.75, 0.2)]	
E- Team (Priority 2)		
No crews are selected.		
- E Spare Part Pool		
<u>⊨</u> - Pool	Pump Gland Reconditioning Kit (\$3000)	
— Spares in pool	Unlimited	
 Logistic time for spare acquisition 	Default - Immediate Availability	
Quantity requested by task	1	
Task Consequences		
+ 2 Restoration		~
Us	ed by 3 items 🔣 🖉 OK	Cancel
Local Resource	Editing corrective task	properties

- As you can see, the task includes the following properties:
 - The "Emergency Repack" corrective task will be performed upon item failure and the task duration is 3 hours.
 - When the pump has to be correctively repaired, there is a delay before the emergency maintenance (EM) crew can respond, and the cost for their time is \$200 per hour. The "Pump Gland Reconditioning Kit" used to repair the pump costs \$3,000.
- Click **Cancel** to close the window without saving any changes.

View the Maintenance Task Selection

The Tasks node in the FMEA hierarchy provides access to the tools available in RCM++ to assist with maintenance task selection. It also displays the maintenance tasks that have been defined in the analysis for a particular failure mode.

• To open the Task Manger window for the "Wear Out - Normal wear" failure mode, doubleclick the **Tasks** node under that record.

- 🖓 Wear Out - Normal wear	
占 Reliability Policy - Wear Out - Normal wear	
📰 CM - RR - Packing Gland Asm	
Wear Out - Normal - Model [WB2 (3.5, 8500)]	
- Tasks	

The top section of the Task Manager window displays the failure effect categorization for this failure mode, along with the maintenance task selection questions that are applicable for that FEC. (This is based on the configurable maintenance task selection logic that has been defined for all RCM analyses in the current project.)

You can see that the team has indicated that a scheduled restoration task (i.e., a planned preventive maintenance) may be applicable and effective to address this potential failure mode.

🛞 Task	Manager											×
			×.	R		6			S			
Add Task	Add Existing Tasks	Edit Task	Delete Task	Edit URD	Edit Mode		Corrective Task	Effect Categorization	Simulat	e		
	Tasks	5			Related F	Records		Tools				
FEC: 2 - Ev	ident Econon	nic Conseq	uences									
		Questi	on			Yes/No		Ex	planati	on		
4: Is a sche doing?	duled on-cond	lition task t	echnically	/ feasible an	d worth	No						
5A: Is a scl doing?	neduled restor	ation task t	echnically	feasible an	d worth	Yes						
5B: Is a sc doing?	neduled discar	d task techi	nically fea	sible and w	orth	No						
Run to Fai	lure:		Cost per	Operating	Time 1.5	399		Availat	oility ().9996		
Tasks												
	Name		Туре	Operatin	g Cost Co	ost per O	perating 1	lime 🛛	Av	ailability		_
L									[:			
										OK	Cano	el
Task Mana	ger											:

• The preventive maintenance task that the team wants to consider for this issue has already been saved as a resource in the sample database. To select it, choose Add Existing Tasks.



• The Select Resource window displays a list of all the scheduled maintenance tasks that have already been created for this project. Select **PM - RR - planned pump** and click **OK**.

		• 🗟 🖶 -		Select Resource		• ×
Но	ome	Administration				•
Sho	w All	Show Only Show Only	how Global	Duplicate - U	ace Make Global age	
Sho	w All					• + / ×
		Task Name	Task Type	Task Frequency	Action Duration	Duration Model Information
Ŧ		RBC	RBC	RBC	RBC	RBC
2		Inspect for broken / damaged i	Inspection (IN)	Fixed time interval based on calendar t	ime Impeller inspection wear / corros	NOR (0.5, 0.1)
2		Training; Maintenance - Proper	Training (Tra)	Fixed time interval based on calendar t	ime Training Week	40
9		PdM - Track Flow Rate	PdM - Online Monitoring (OLM)	Fixed time interval based on calendar t	ime Flow Rate Tracking	NOR (0.25, 0.1)
2		OC- Inspection for corrosion	Condition Based (OC)	Fixed time interval based on item age	Impeller inspection wear / corros	NOR (0.5, 0.1)
2		PM - Gland Follower	Repair/Replace (RR)	Fixed time interval based on calendar t	ime PM - Gland Follower	NOR (3, 1)
: 💡		IN - Inspection for leaks	Condition Based (OC)	Fixed time interval based on calendar t	ime OC-Inspection	NOR (0.25, 0.1)
2	\checkmark	PM - RR - planned pump	Repair/Replace (RR)	Fixed time interval based on calendar t	ime Planned Repack and Condition	1.5
2		Training; Maintenence	Training (Tra)	Fixed time interval based on item age	Training Week	40
•						•
					OK	Cancel
Scho	eduled	Tasks Show Local Resources	All			

• Notice that the task is now visible in the Tasks section of the Task Manager window. Double-click the task to view its properties.

Task Name	Task Type	
PM - RR - planned pump	Repair/Replace (RR)	
•		
ask Properties		
🖬 🛃 Task Scheduling		
— When is this task performed?	Fixed time frame based on calendar time	•
 Fixed interval 	1	
— Unit	Hour (hr)	•
Override task scheduling properties wit	h a task package	
🛛 🏠 Basic Task Properties		
- 🔼 Task duration (hr)	Planned Repack and Condition [1.5]	
🕂 📇 Teams for task		
- Team (Priority 1)		
- Crew	PM Crew \$180/Hr	
– Logistic delay	Default - Immediate Availability	
⊢ Team (Priority 2)		
No crews are selected.		
占 📲 Spare Part Pool		
E- Pool	Pump Gland Reconditioning Kit (\$3000)	
— Spares in pool	Unlimited	
 Logistic time for spare acquisition 	Default - Immediate Availability	
Quantity requested by task	1	
Task Consequences		
댙 II 🕨		
Use	ed by 1 item	Cancel

As you can see, the spare parts logistics are the same as they were for the corrective maintenance. Notice, however, that the repair time duration is only 1.5 hours and that the planned maintenance (PM) crew is less expensive (as it is only \$180 per hour).

You will also notice that the scheduled task interval is temporarily set to 1 as a placeholder for the actual value. You can use the Failure Modes and Reliability Analysis (FMRA) interface to calculate the optimum replacement time. The FMRA interface is available in multiple ReliaSoft

applications (including BlockSim, XFMEA and RCM++) and it facilitates a variety of system reliability, availability and maintainability calculations.

- After you are done viewing the properties, close the Maintenance Task and the Task Manager windows.
- To display the FMRA for the sample project, View > Show > Show FMRA.



• With the system item selected, open the Optimum Replacement window by choosing **FMRA > Calculations > Optimum Replacement**.



The Optimum Replacement window displays all of the maintenance tasks that are defined in the current project. You can choose to calculate the optimum replacement time for a single task, or you can select multiple tasks to optimize together. For this example, you will perform the calculation for a single task, where the planned replacement cost is \$6,320 and the unplanned replacement cost is \$11,300.

- Select the **Wear Out Normal wear** failure mode and enter the planned replacement cost and the unplanned replacement cost.
- Click Calculate to open the Optimum Replacement Calculations window. Choose the Individual Blocks can use different times option, then click OK. In the Optimum Replacement window, notice that the Optimum Replacement Time column now shows the calculated result of ~7,116 hours.

٠	*				()ptimum Repl	acement			□ ×
Delete	Cut	Displa		Clear	βη σμ Calculate	Cost vs. Crea	te Maintena	nce		
	Paste	Parent I	tem	Values	1	Fime Plot	Task(s) *			
	Edit	Preferer	ices	Costs		Tools				
V	Available Items Packing Gland	too tigh		Iten	n Name	Planned Replacement		Unplanned eplacement Cost	Optimum Replacement Time (hr)	Replacement Cost per Unit Time (hr)
	Induced - Inco		\rightarrow	Wear Out	- Normal wear	6320		11300	7115.3698	1.3147
	Wear Out - No Induced - Pack Induced - Glan Induced - Glan Vane wear Broken impeller Key - Coupling Lock nut Assen Key - Impeller	ing nut Id Follow Id Follow r vane mbly - sh	Peel	account Coo	t Dar I Jait Tima	(her)				
	Slinger Ring - v Wear plate	water	Repla	acement Cos	t Per Unit Time	(hr) 1.3147				

- Close the Optimum Replacement window, then return to the system hierarchy view and click the **FMEA** tab to open the FMEA.
- Open the Task Manager window, then open the "PM RR planned pump" task and enter the calculated time in the **Fixed interval** field.

🖃 🛃 Task Scheduling		
— When is this task performed?	Fixed time frame based on calendar	time 🔹 🔻
 Fixed interval 	7116	
— Unit	Hour (hr)	•
Override task scheduling proper	ties with a task package	

• Close the Maintenance Task window, and then click **Simulate** in the Task Manager window to determine which maintenance strategy (run-to-failure or preventive maintenance) will provide better results.



• When prompted, accept the simulation value for the hours of operation (20,000), and select to run 1,000 simulations and then click **OK**. When the simulation is complete, the run-to-failure (corrective maintenance only) results are displayed above the table and the results for the preventive maintenance strategy are displayed with the task. As you can see, the availability is very similar between the run to failure and PM options, but the cost per operating

time is less when using PM. For a mission of 20,000 hours, this will result in significant cost savings.

🛞 Task	Manager											×
			×.	R					S			
Add Task	Add Existing Tasks	Edit Task	: Delete Task	Edit URD	Edit Mod		Corrective Task	Effect Categorization	Simulate			
	Tasks	5			Related	Records		Tools				
FEC: 2 - Ev	ident Econon	nic Conse	quences									
		Quest	ion			Yes/No		Exp	lanation	n		
4: Is a sche doing?	duled on-cond	lition task	technically	feasible an	d worth	No						
5A: Is a sch doing?	eduled restor	ation task	technically	feasible an	d worth	Yes						
5B: Is a sch doing?	neduled discar	d task tec	hnically fea	sible and wo	orth	No						
Run to Fai	lure:	ſ	Cost per	Operating	Time 1.5	300		Availab	oility 0.9	9996		
Tasks												
	Name		Туре	Operatin	g Cost C	ost per O	perating	Time	Ava	ilability		
PM - RR - p	lanned pump		RR	2.1297E	+04	1	.0648		0	.9997		
									0	Ж	Cano	el
Task Manag	jer											

• Click **OK** to close the window.

Calculate System Reliability and Availability

Return to the FMRA view so you can simulate the entire system and calculate the availability with the potential failure modes and maintenance tasks that are currently specified.

• To select which columns in the FMRA to show on your computer, right-click a column header in the FMRA and choose **Customize Columns**. Enable only the fields that are shown in the following picture (**Reliability Policy**, **Simulation Results Status**, **Operating Cost**, **Cost per Operating Time** and **Availability**), then **click** OK.

Column	Description	^
Reliability Policy	How the reliability will be calculated (inherit, default or the name of the URD).	
Mirror Groups	Indicates whether the cause is a member of a mirror group.	
Analytical Results Status	Green when analytical results are current, red when they are not current.	
Target Reliability	Target Reliability	
Reliability (Analytical)	Displays the record's calculated reliability at the system's specified operating time.	
Probability of Failure (Analytical)	Displays the record's probability of failure at the system's specified operating time. This is the inverse of reliability (1-R).	
✓ Mode Ratio	Normalized mode ratio of the item's probability of failure (for criticality analysis).	
✓ Prob of Loss	Displays a factor from 0 to 1 that describes the probability that this failure mode would result in a system failure.	
Criticality	Displays the calculated criticality value. (This column must be displayed when the mode ratio or probability of loss is displayed.)	
Simulation Results Status	Green when simulation results are current, red when they are not current.	
Operating Cost	Displays the total costs that accrued during the simulation.	
Cost per Operating Time	Displays the operating cost divided by the total operating time.	
TargetAvailability	TargetAvailability	
✓ Availability	Displays the average availability (i.e., uptime divided by total operating time).	.

• To give more space in the System panel before calculating the costs, choose View > Workspace Layout > Hide Analysis Panel.



• Choose FMRA > Calculations > Simulate (Availability).

• Use the same operating time of 20,000 hours and the same number of simulations (1,000), and then click **OK**. The calculated results are shown next.

📩 System Hierarchy					
Name	Reliability Policy	F	Operating Cost	Cost per Operating Time	Availability
🛛 💼 Pump_Centrifugal_MotorDrive	Inherit		3.7202E+05	18.6012	0.9150
⊨ ▶ Move a given fluid while maintaining an accepta	Inherit		1.1000E+05	5.5002	0.9994
🖃 🗙 Functional Failure: Ext. leak at input shaft	Inherit		7.1363E+04	3.5682	0.9997
- ? Packing Gland too tight / loss of lubrication	Induced - Packing Gland too tight / lo		2.5830E+04	1.2915	1.0000
- ? Induced - Incorrect installation	Induced - Incorrect installation		2.4870E+04	1.2435	1.0000
🖓 Wear Out - Normal wear	Wear Out - Normal wear		2.0664E+04	1.0332	0.9997
= 🗙 Functional Failure: Leak rate at the Shaft is b	Inherit		2.4757E+04	1.2378	1.0000
Induced - Packing nut over tightened	Operator error- packing set-up		2.4757E+04	1.2378	1.0000
⊢× Functional Failure: Catastrophic failure of the	Inherit		1.3884E+04	0.6942	0.9997
- ? Induced - Gland Follower corrosion / failure	Gland Follower corrosion / failure		1.2963E+04	0.6481	0.9998
Induced - Gland Follower stress / failure	Gland Follower stress / failure		921.5216	0.0461	1.0000

You can see that the estimated availability with the current maintenance strategy is about 92% and the cost per operating time is \$18.60. For a period of 20,000 hours, that is a total operating cost of approximately \$372,024. Packaging the tasks into more efficient intervals may provide better results, as discussed next.

Using Task Packaging

For a given project, you can use the Scheduled Task Packaging window to review all of the tasks that have been proposed to be performed at fixed intervals, choose which ones to incorporate in the final maintenance plan and, if desired, group tasks into packages for the most efficient allocation of resources.

• Return to the system hierarchy, then choose System Hierarchy > Tools > Task Packaging.



This utility provides several flexible tools to help you select the most effective maintenance packaging plan. For this example, you will use the time clusters feature, which automatically groups tasks into a specified number of intervals.

• Under "Time - Clusters" enter **3** and click **Time - Clusters**. The utility will automatically propose the three packages shown next.

Scheduled Task Packaging (Project: RCM -	Pump	Analysis wit	h Simulation	5)							>
The - Cluster	rs	🚺 Ungroup S	elected	× Re	emove Level			٥		0	
Type Zone Access 🎉 🔒	:	🗙 Delete Em	pty Packages	ී St	art Over	Tools		lpdate kages *		Display	
Group By			Manage	Groups							
Description	Flag	Task Type	Start Interv	al (hr)	Interval (hr)	End Inter	val (hr)	Zone	Access	i Sta	atus
- 漪 Interval: 730 - 2190			730		1309	219	90				
- PdM - Track Flow Rate		PdM - Online Monitoring			730						
— IN - Inspection for leaks		Condition Based			1008						
Inspect for broken / damaged impeller vane		Inspection			2190						
🛚 🎁 Interval: 7116 - 12650			7116		9322	126	50				
— PM - RR - planned pump		Repair/Repl ace			7116						
 Training; Maintenance - Proper Packing 		Training			8760						
 Training; Maintenence 		Training			8760						
OC- Inspection for corrosion		Condition Based			12650						
🗆 🎁 Interval: 330000 - 330000			33000)	330000	3300	00				
PM - Gland Follower		Repair/Repl ace			330000						
Tasks Plot					-						

• Click the **Update Packages > Apply Changes** command on the ribbon to create these packages in the database to automatically override the task intervals for the affected maintenance tasks.



• Close the window, then return to the FMRA and simulate the results again. You can see that the availability is now around 93% and that the cost per operating time has decreased to \$7.15. For a period of 20,000 hours, that is a total operating cost of approximately \$143,078.

System Hierarchy				
Name	Reliability Policy	Operating Cost	Cost per Operating Time	Availability
🖃 💼 Pump_Centrifugal_MotorDrive	Inherit	1.4308E+05	7.1539	0.9325
⊨ ▶ Move a given fluid while maintaining an accepta	Inherit	1.1980E+05	5.9898	0.9914
+X Functional Failure: Ext. leak at input shaft	Inherit	7.8569E+04	3.9285	0.9925
-? Packing Gland too tight / loss of lubrication	Induced - Packing Gland too tight / lo	2.5839E+04	1.2920	1.0000
- 7 Induced - Incorrect installation	Induced - Incorrect installation	2.4951E+04	1.2476	1.0000
🖓 Wear Out - Normal wear	Wear Out - Normal wear	2.7779E+04	1.3889	0.9926
-X Functional Failure: Leak rate at the Shaft is b	Inherit	2.4815E+04	1.2407	1.0000
Induced - Packing nut over tightened	Operator error- packing set-up	2.4815E+04	1.2407	1.0000
⊢× Functional Failure: Catastrophic failure of the	Inherit	1.6412E+04	0.8206	0.9976
- ? Induced - Gland Follower corrosion / failure	Gland Follower corrosion / failure	1.5502E+04	0.7751	0.9976
Induced - Gland Follower stress / failure	Gland Follower stress / failure	909.7758	0.0455	1.0000

• To see what the results would be if there were four packages, return to the Task Packaging window. Select each package and click **Ungroup Selected**.



• When all of the tasks are back to being unassigned, click **Delete Empty Packages** to clear the old groupings.



- Set the number of packages to 4 and click **Time Clusters** to automatically regroup the tasks into four packages.
- Click Apply Changes to save the new packages and override the task intervals.
- Close the window, then return to the FMRA and simulate the results again. You can see that the availability is now around 92%, and the cost per operating time has decreased to \$6.79. For a period of 20,000 hours, that is a total operating cost of approximately \$135,710.

🕂 System Hierarchy				
Name	Reliability Policy	Operating Cost	Cost per Operating Time	Availability
Pump_Centrifugal_MotorDrive	Inherit	1.3571E+05	6.7855	0.9222
+ Move a given fluid while maintaining an accepta	Inherit	1.1265E+05	5.6327	0.9935
-X Functional Failure: Ext. leak at input shaft	Inherit	7.3463E+04	3.6731	0.9937
- ? Packing Gland too tight / loss of lubrication	Induced - Packing Gland too tight / lo	2.5791E+04	1.2895	1.0000
- ? Induced - Incorrect installation	Induced - Incorrect installation	2.4957E+04	1.2479	1.0000
🖓 Wear Out - Normal wear	Wear Out - Normal wear	2.2715E+04	1.1357	0.9938
-X Functional Failure: Leak rate at the Shaft is b	Inherit	2.4800E+04	1.2400	1.0000
Induced - Packing nut over tightened	Operator error- packing set-up	2.4800E+04	1.2400	1.0000
⊢× Functional Failure: Catastrophic failure of the	Inherit	1.4392E+04	0.7196	0.9997
- ? Induced - Gland Follower corrosion / failure	Gland Follower corrosion / failure	1.3529E+04	0.6765	0.9997
Induced - Gland Follower stress / failure	Gland Follower stress / failure	863.0519	0.0432	1.0000

• You can continue to experiment with the cost and availability calculations, if desired. When finished, proceed to the next section.

Generate a Report of the Analysis

RCM++ provides a complete set of reports for your analysis. Reports can be generated in Microsoft Word® and/or Excel, which provides maximum flexibility for customization and the ability to create HTML and/or PDF versions of the reports.


• To open the Reports window, choose **Home > Reporting > Reports**.



- The Select Items area (on the left) allows you to specify the item(s) from the system hierarchy that will be included in the report. Make sure that all seven items are selected.
- The Available Reports area (in the middle) displays the report forms that are available to be included in the report document, while the Selected Reports area (on the right) displays the report forms that will be included in the new report you are generating now. Click the Exclude All icon (<<) to clear the Selected Reports area so you can start building the new report from scratch.
- In the Available Reports area, press **CTRL** and click each of the following report forms so they are all selected at the same time.
 - Under the Risk Discovery heading, select Risk Discovery Details (One per Item).
 - Under the RCM heading, select:
 - Functional Failure Analysis
 - Failure Effect Categorization (One per Effect)
 - Maintenance Task Selection (One per Cause)
 - Tasks
- Click the **Select** (>) icon to move all five of these report forms into the Selected Reports area.

Tip: You can also drag and drop or double-click the report form names to move them back and forth between "available" and "selected."

• Finally, select to generate the report as an **Excel Spreadsheet**. The Reports window will look like the one shown next.

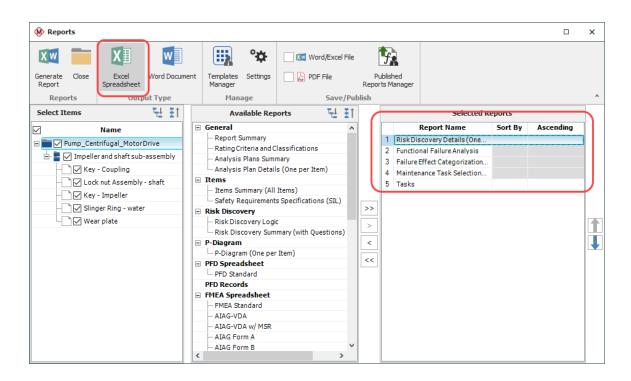

• Click Generate Report and specify a name and location for the document. When you click Save, a progress bar will appear. After the report is complete, it will open automatically in Microsoft Excel. When you are finished reviewing the reports, close Excel and the Reports window.

Close the Database

Congratulations! You have completed the First Steps Example for RCM++.

• To close the sample database, choose **File > Close Database**.

Note that if you do not close the database, it will be closed automatically when you create or open a new one.